


Purified anti-Cytokeratin, HMW Antibody

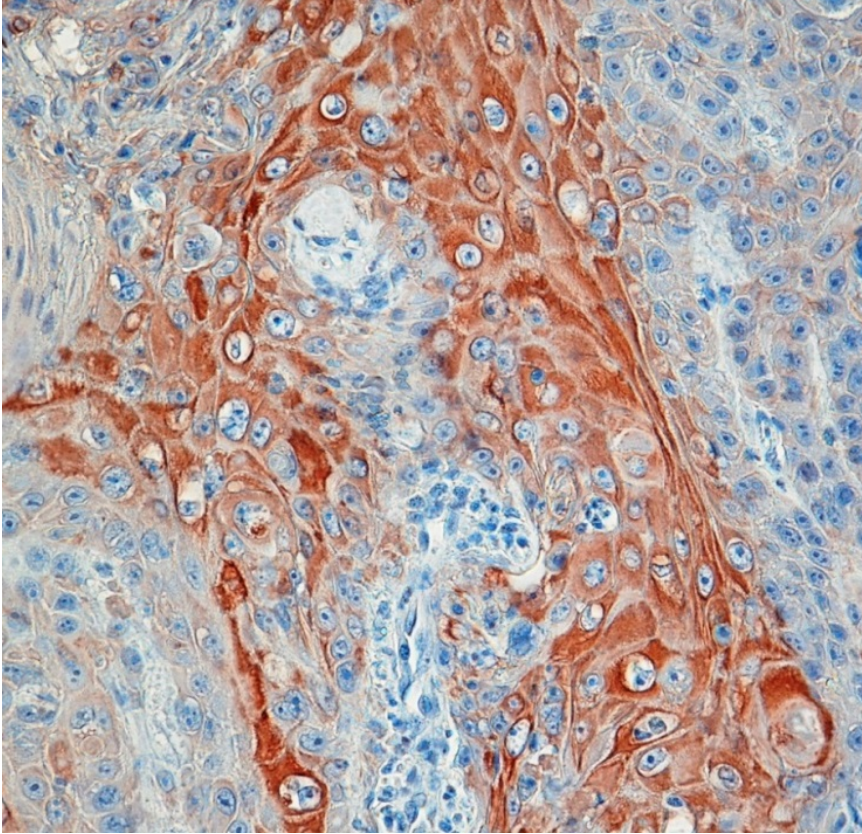

IHC staining of anti-Cytokeratin, HMW antibody (clone 34 β E12) on formalin-fixed paraffin-embedded normal human skin. After antigen retrieval using Retrieve-All Antigen Unmasking System 1, the tissue was incubated with the primary antibody at 0.7 μ g/ml for 60 minutes at room temperature. BioLegend's Ultra Streptavidin (USA) HRP Detection Kit was used for detection followed by hematoxylin counterstaining.